



US00D765835S

(12) **United States Design Patent** (10) **Patent No.:** **US D765,835 S**
Kammer et al. (45) **Date of Patent:** **** Sep. 6, 2016**

(54) **CONTAINER FOR FORMATION OF SURGICAL SLUSH**

(71) Applicant: **C° Change Surgical LLC**,
Winston-Salem, NC (US)

(72) Inventors: **Patrick Kammer**, Greensboro, NC (US); **Kevin Joseph Rackers**,
Summerfield, NC (US)

(73) Assignee: **C° Change Surgical LLC**,
Winston-Salem, NC (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/510,524**

(22) Filed: **Nov. 30, 2014**

(51) **LOC (10) Cl.** **24-04**

(52) **U.S. Cl.** **D24/121**
USPC

(58) **Field of Classification Search**
USPC D24/121, 113, 112, 127, 224, 117;
604/403; D9/453, 449, 447, 440, 436,
D9/435, 434, 516, 547, 549, 560, 572,
D9/573; D7/398, 397, 608, 602, 619.1,
D7/629; 222/570, 569, 544, 548, 562, 157,
222/158
CPC .. A61B 19/081; A61F 7/0241; A61F 7/0085
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,809,068 A * 5/1974 Kosowsky A61B 5/1405
422/913
- D335,450 S * 5/1993 Pezzoli D24/197
- D337,271 S * 7/1993 Pezzoli D9/453
- D354,913 S * 1/1995 Pezzoli D24/197
- D439,345 S * 3/2001 Herchenbach D24/224

- D471,101 S 3/2003 Bezek
- D533,670 S * 12/2006 Py D24/121
- D537,721 S * 3/2007 Kertels D9/449
- H2199 H 9/2007 Horton
- D559,396 S * 1/2008 Dave D24/121
- D561,908 S 2/2008 Py
- D569,195 S 5/2008 Kim
- D592,909 S * 5/2009 Alviar D7/510
- D627,604 S 11/2010 Eyal

(Continued)

OTHER PUBLICATIONS

C Change Surgical website, Intelli-Slush, Feb. 3, 2015, <http://www.cchangesurgical.com/surgislush.html>.*

(Continued)

Primary Examiner — David Muller

Assistant Examiner — Nathan Johnston

(74) *Attorney, Agent, or Firm* — Kevin E. Flynn; Flynn IP Law


(57) **CLAIM**

The ornamental design for a container for formation of surgical slush, as shown.

DESCRIPTION

FIG. 1 is a perspective view of the right side, front side, and top side of a container for formation of surgical slush with a container top showing the new design; FIG. 2 is a perspective view of the right side, front side, and top side of a container without the container top of FIG. 1; FIG. 3 is a front side elevational view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is a left side elevational view thereof; and, FIG. 6 is a rear side elevational view thereof. The broken lines are shown for environmental purposes only and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

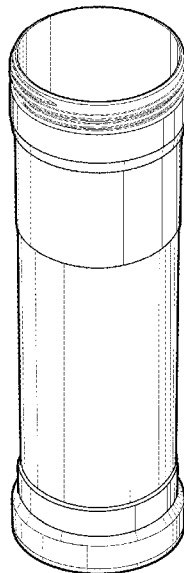

(56)

References Cited

U.S. PATENT DOCUMENTS

7,874,167	B2	1/2011	Kammer	
D641,591	S *	7/2011	Tsukida	D7/608
D652,682	S *	1/2012	Eyal	D7/510
D690,161	S	9/2013	Garner	
D709,734	S *	7/2014	Kotani	D7/608
D729,584	S *	5/2015	Weston	D7/510
D729,585	S	5/2015	Boroski	
D741,655	S	10/2015	Whelan	
D744,781	S	12/2015	Rummel	
2010/0200602	A1	8/2010	Chan	

OTHER PUBLICATIONS

C Change Surgical Facebook, Intelli-Slush, Jan. 18, 2015, <https://www.facebook.com/SurgiSlush-315075491944248/>.
 * 1000 mL Standard Jar, web page found at <http://www.savillex.com/ProductDetail.aspx?ProductName=Jar-only-1000-ml-threaded-top>, copyrighted 2013, Savillex Corporation, Eden Prairie, MN, USA.
 Jar Dimensions, PDF file linked to web page found at <http://www.savillex.com/ProductDetail.aspx?ProductName=Jar-only-1000-ml-threaded-top>, PDF metadata indicates file creation date of Nov. 28, 2012, Savillex Corporation, Eden Prairie, MN, USA.

* cited by examiner

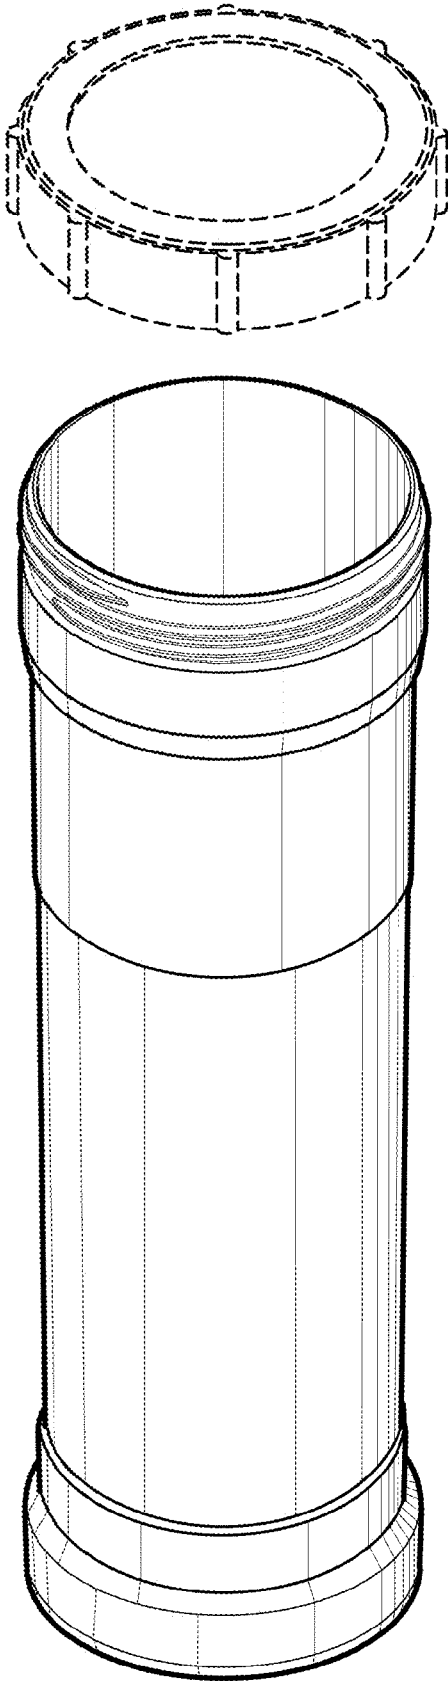


FIG. 1

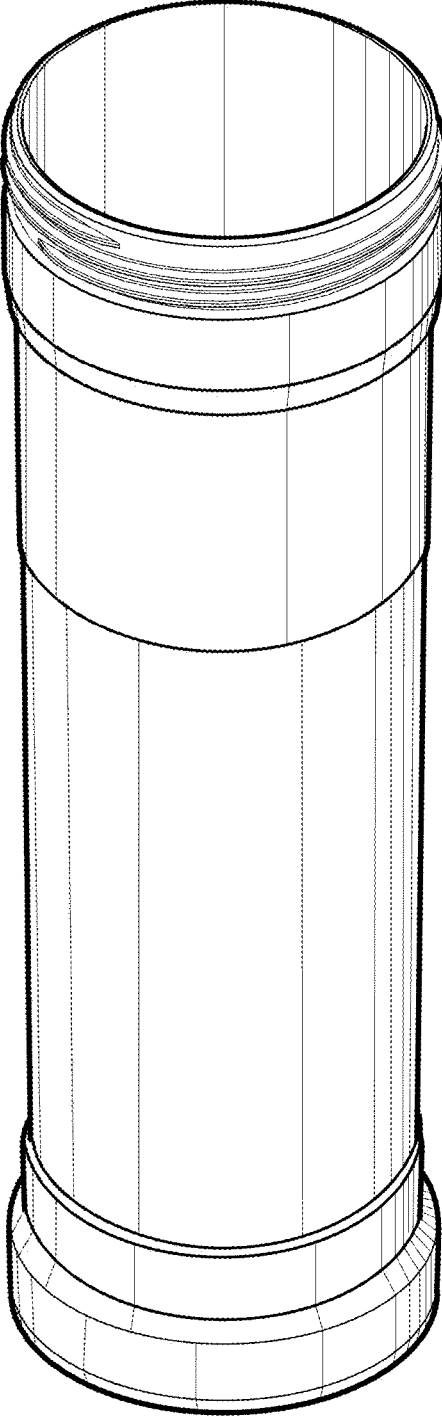


FIG. 2

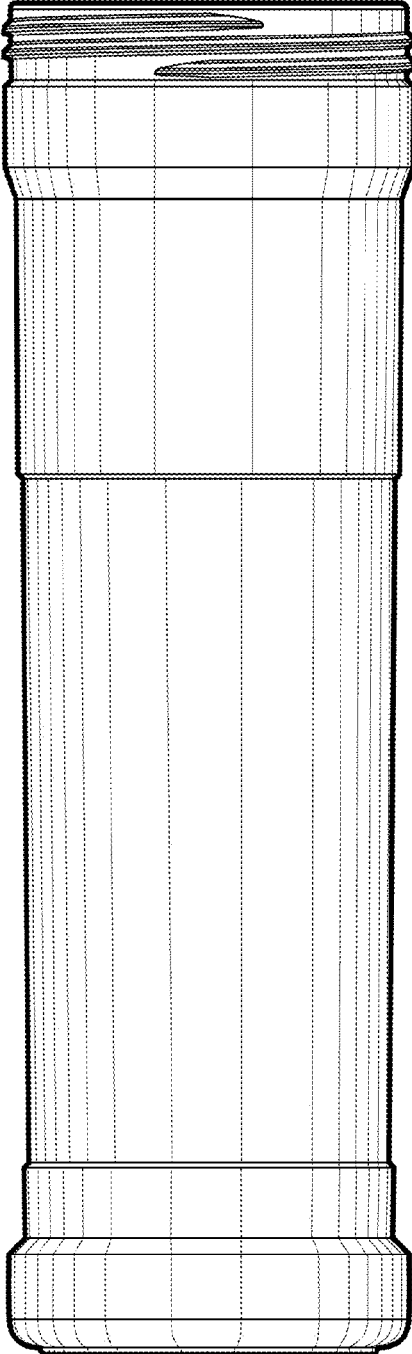


FIG. 3

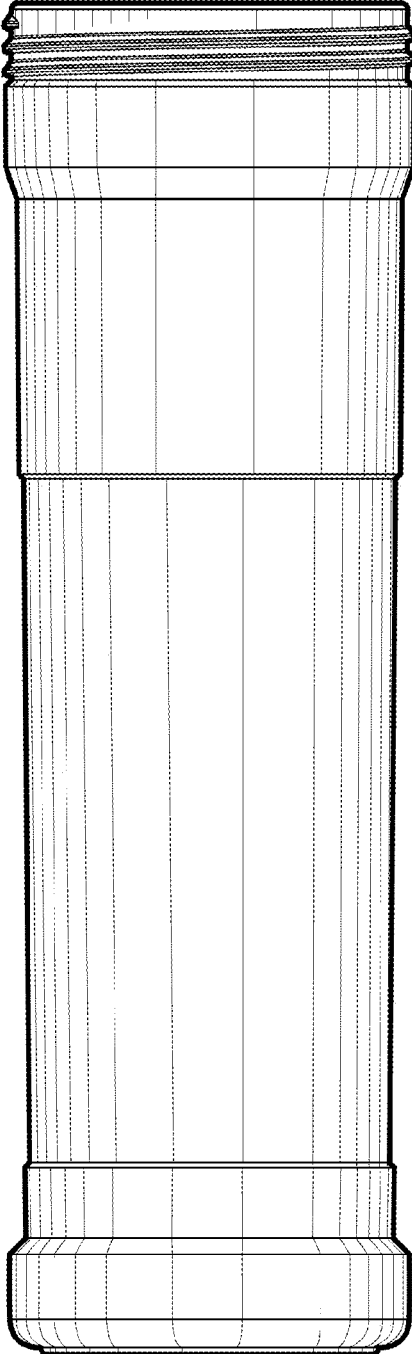


FIG. 4

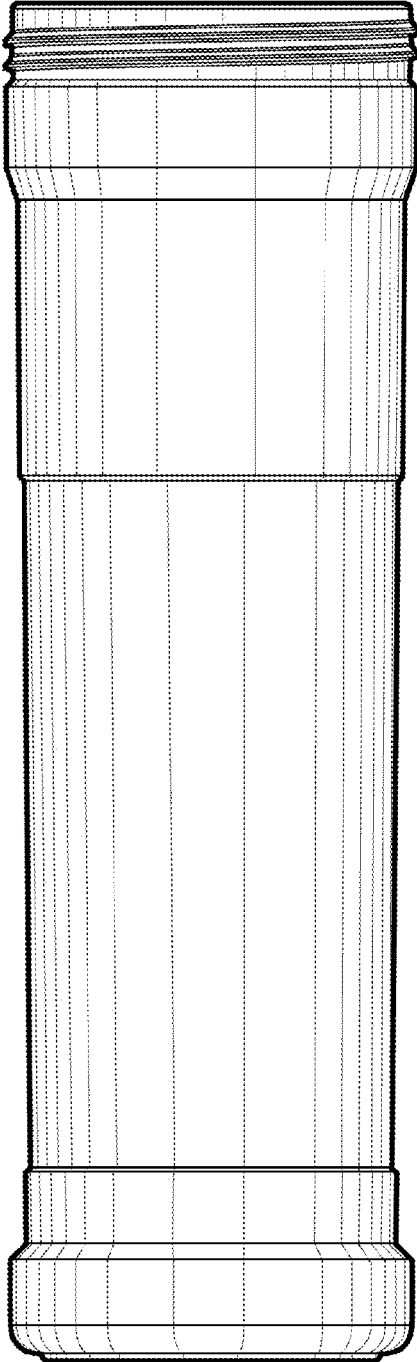


FIG. 5

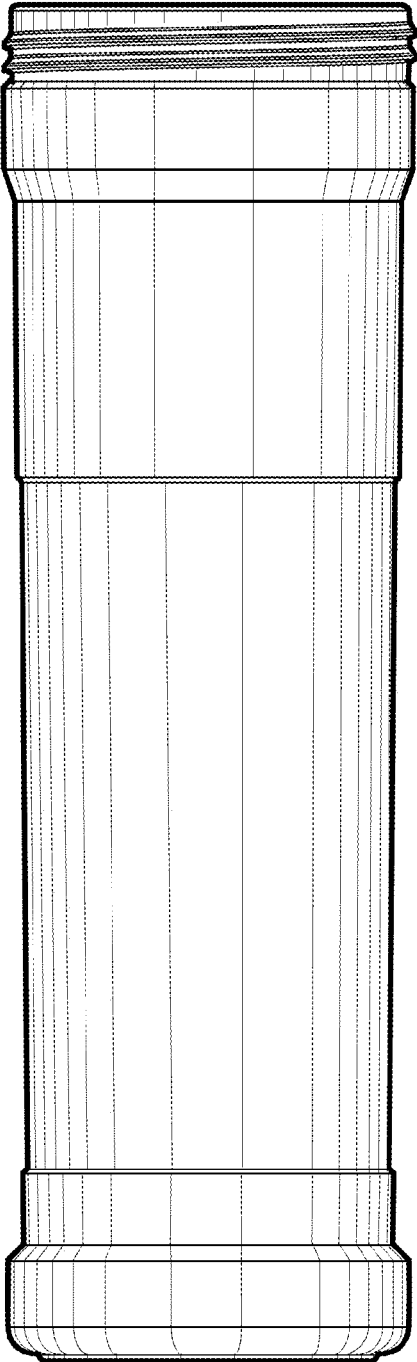


FIG. 6